ЗАКАЗАТЬ: CO-AX Alphasense сенсор угарного газа 0-2000 ppm

CO-AX/CO-AX+ Carbon Monoxide Sensor – Low Hydrogen Cross Sensitivity

The CO-AX sensor is a PPM sensor that is designed for a broad variety of applications and instrumentation including portable gas detectors and fixed gas detection systems for industrial safety, environmental air quality analysis and process control. The A series is the most widely used sensor format for portable gas detection applications. It is available in our standard format (CO-AX) and with our patented Integrated Smart Technology (CO-AX+) that has an IST board with a memory chip and temperature sensor integrated in the sensor. The + sensors store specific calibration, specification, and identification data on every sensor allowing plug and play operation. The on-board temperature sensor improves the accuracy and simplicity of temperature compensation algorithms.

CO-AX Carbon Monoxide Sensor – Low Hydrogen Cross Sensitivity – 3-Electrode

Top View

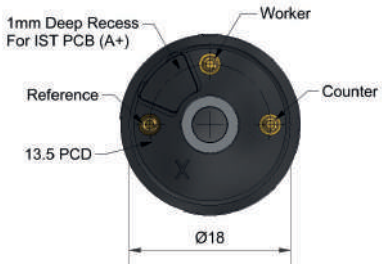

Bottom View

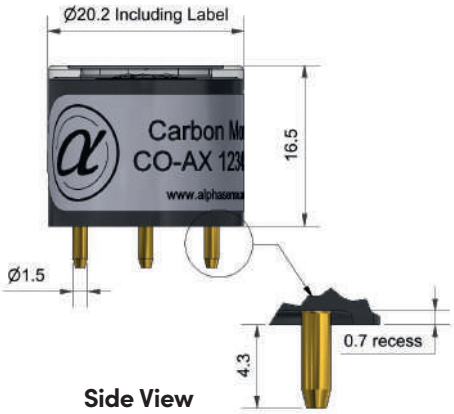

Side View

CO-AX+ Carbon Monoxide Sensor – Low Hydrogen Cross Sensitivity – 3-Electrode (with Integrated Smart Technology)

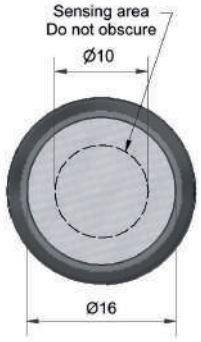

Top View

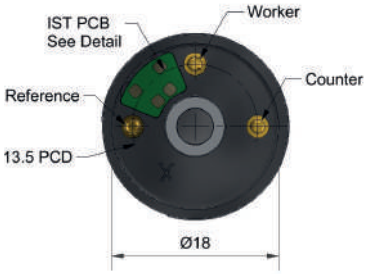

Bottom View

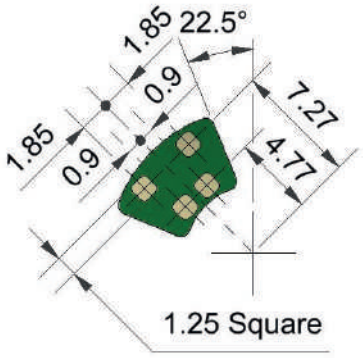

IST Board

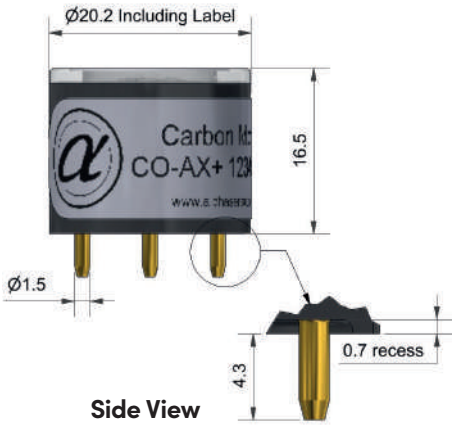

Side View

Dimensions are in millimetres (± 0.15 mm).

Sensor Data

Performance	Sensitivity	nA/ppm in 400ppm CO		55 to 100
	Response time	t90 (s) from zero to 400ppm CO		< 30
	Zero current (typical)	ppm equivalent in zero air		< ± 3
	Resolution	RMS noise (ppm equivalent)		< 0.5
	Range	ppm CO limit of performance warranty		2,000
	Linearity	ppm error at full scale, linear at zero and 800ppm CO		< ± 40
	Overgas limit	maximum ppm for stable response to gas pulse		4,000
Lifetime	Zero drift	ppm equivalent change/year in lab air		< 0.2
	Sensitivity drift	% change/year in lab air, monthly test		< 6
	Operating life	months until 80% original signal (24-month warranted)		> 24
Environmental	Sensitivity @ -20°C	(% output @ -20°C/output @ 20°C) @ 400ppm CO		55 to 75
	Sensitivity @ 0°C	(% output @ 0°C/output @ 20°C) @ 400ppm CO		75 to 90
	Sensitivity @ 40°C	(% output @ 40°C/output @ 20°C) @ 400ppm CO		106 to 120
	Zero @ -20°C	ppm equivalent change from 20°C		< 0 to 4
	Zero @ 0°C	ppm equivalent change from 20°C		< 0 to 3
	Zero @ 50°C	ppm equivalent change from 20°C		< 0 to -6
Cross Sensitivity	Filter capacity	ppm·hrs	H_2S	250,000
	Filter capacity	ppm·hrs	NO_2	500,000
	Filter capacity	ppm·hrs	NO	20,000
	Filter capacity	ppm·hrs	SO_2	250,000
	H_2 sensitivity	% measured gas @ 900ppm	H_2 in 900ppm CO @ 10°C	< 2
	H_2 sensitivity	% measured gas @ 900ppm	H_2 in 900ppm CO @ 20°C	< 4
	H_2 sensitivity	% measured gas @ 900ppm	H_2 in 900ppm CO @ 30°C	< 6
	NO_2 sensitivity	% measured gas @ 10ppm	NO_2	< -1
	Cl_2 sensitivity	% measured gas @ 10ppm	Cl_2	< 0.1
	NO sensitivity	% measured gas @ 500ppm	NO	< -2
	SO_2 sensitivity	% measured gas @ 20ppm	SO_2	< 0.1
	C_2H_4 sensitivity	% measured gas @ 400ppm	C_2H_4	< 5
	NH_3 sensitivity	% measured gas @ 20ppm	NH_3	< 0.1
Key Specifications	Temperature range	°C		-30 to 50
	Pressure range	kPa		80 to 120
	Humidity range	% rh continuous		15 to 90
	Storage period	months @ 0 to 20°C (stored in sealed pot)		6
	Load resistor	Ω (recommended)		10 to 47
	Weight	g		< 6

Figure 1 CO Sensitivity Temperature Dependence

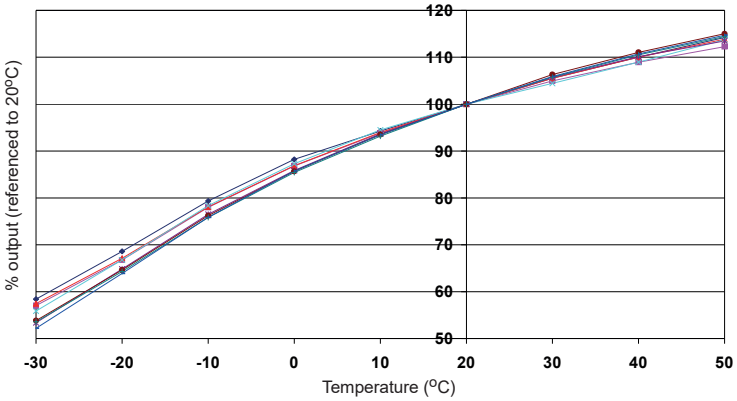

Figure 1 shows the variation in sensitivity caused by changes in temperature.

This data is taken from a typical batch of sensors.

Figure 2 Hydrogen Sensitivity Temperature Dependence

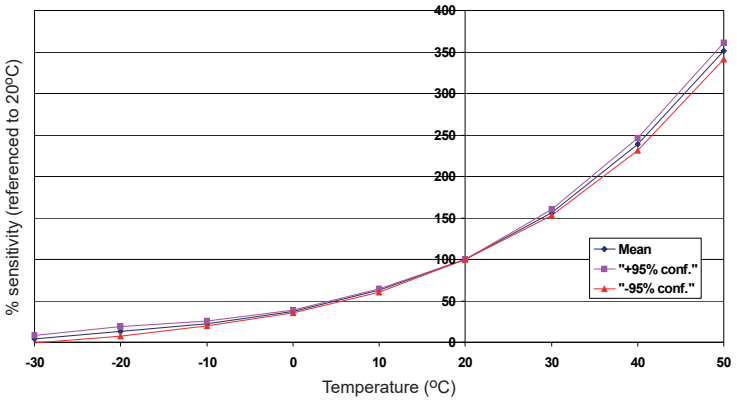

Figure 2 shows the strong temperature dependence of the CO-AX to hydrogen. Since hydrogen sensitivity is less than 4% at 20°C, hydrogen interference can practically be ignored at low temperatures. However, at 50°C hydrogen interference is 14%.

This data is taken from a typical batch of sensors. The mean and ±95% confidence intervals are shown.

Figure 3 Hydrogen Cross Sensitivity at 30°C

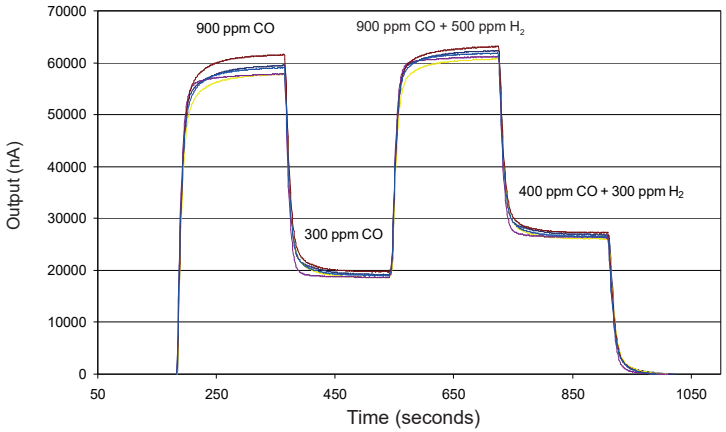

Figure 3 shows hydrogen sensitivity for a typical batch of eight CO-AX sensors at 30°C following EN50379. All sensors show less than 5% cross sensitivity when 500ppm hydrogen is added to 950ppm carbon monoxide. t90 is less than 45 seconds.

IST Board Data

Interface	Communication Bus	Compatible with the 400 kHz I²C protocol
	Max. Bus Speed	Up to 1 MHz
	Input Logic Levels	High (Recessive) < 2.3 V | Low (Dominant) < 0.2 V
	Absolute Max. Input Signal	3.6 V
Electrical	Supply Voltage Range	1.7 V to 3.6 V
	Supply current – Stand-By	< 5 µA
	Supply current – Operating	< 0.15 mA (temperature reading only) < 2.15 mA (temperature reading + memory reading/writing)
	Power Supply Conditioning	Built-In 100 nF decoupling capacitor
	ESD Protection	4 kV (human body model) - Enhanced ESD / Latch-Up protection
	Bus Pins Input Capacitance	15 pF max.
Performance	Operational Temperature	–40 °C to +85 °C
	Temperature Sensor Accuracy	±1°C (-0°C to +70°C)
	Memory Data Retention	> 200 years
	Memory Write Cycles	> 4,000,000
Data & Communication	Memory IC & I2C Address	M24128X-FCU | Device Address: R - 0xA0 / W – 0xA1
	Temperature IC & I2C Address	MAX31875R0TZS+T | Device Address: R - 0x90 / W – 0x91
	Product Data Start Address	0x0900
	Calibration Data Start Address	0x0B00
	User Data Area	0x0D00 – 0x18FF (3,072 Bytes)
	CRC Polynomial	0x 01 04C1 1DB7
	Digital Signature Algorithm	SHA-256

Factory-populated data

Product Data
- Data Format Version
- Customer (OEM) ID
- Product ID
- Type of Sensor / Target Gas
- Sensor Serial Number
- End of Storage Period Date
- Sensor Replacement Date
- Product Data Checksum
- Alphasense Digital Signature
- Customer Digital Signature

Calibration
- Calibration Data Units
- Zero (clean dry air) Output
- Calibration Span
- Calibration Output
- Sensitivity
- Calibration Date
- Calibration Data Checksum
- Calibration Data Signature

Sensor Specification
- Over-gas limit
- Concentration Range
- Temperature Range Low
- Temperature Range High
- Humidity Range Low
- Humidity Range High
- Pressure Range Low
- Pressure Range High
- Specification Checksum

15,000+ locations

Customer Specific
- Custom Parameters
- Re-Calibration Due Date
- Operational Limits:
- Low | High | STEL | TWA
- Next Bump Test Due Date
- User Data Area

Important. The CO-AX must be operated with a 0 Volt bias between Reference & Working electrodes. Failure to comply with this requirement will result in a loss of its low Hydrogen cross sensitivity performance.

At the end of the product's life, do not dispose of any electronic sensor, component or instrument in the domestic waste, but contact the instrument manufacturer, Alphasense or its distributor for disposal instructions. NOTE: all sensors are tested at ambient environmental conditions unless otherwise stated. As applications of use are outside our control, the information provided is given without legal responsibility. Customers should test under their own conditions, to ensure that the sensors are suitable for their own requirements.

In the interest of continued product improvement, we reserve the right to change design features and specifications without prior notification. The data contained in this document is for guidance only. Alphasense Ltd accepts no liability for any consequential losses, injury or damage resulting from the use of this document or the information contained within.(©ALPHASENSE LTD) Doc. Ref. CO-AX/SEP24

ЗАКАЗАТЬ: CO-AX Alphasense сенсор угарного газа 0-2000 ppm